

Ackland, T. R., Lohman, T. G., Sundgot-Borgen, J., Maughan, R. J., Meyer, N. L., Stewart, A. D. ... (2012). Current status of body composition assessment in sport: review and position statement on behalf of the ad hoc Research Working Group on Body Composition Health and Performance, under the auspices of the IOC Medical Commission. *Sports Medicine*, 42, 227-249.

Dette er siste tekst-versjon av artikkelen, og den kan inneholde små forskjeller fra forlagets pdf-versjon. Forlagets pdf-versjon finner du på link.springer.com: <http://dx.doi.org/10.2165/11597140-000000000-00000>

This is the final text version of the article, and it may contain minor differences from the journal's pdf version. The original publication is available at link.springer.com: <http://dx.doi.org/10.2165/11597140-000000000-00000>

REVISION 2

Current Status of Body Composition Assessment in Sport

Review and position statement on behalf of the Ad Hoc Research Working Group on Body Composition Health and Performance, under the auspices of the I.O.C. Medical Commission

Timothy R. Ackland¹, Timothy G. Lohman², Jorunn Sundgot-Borgen³, Ronald J. Maughan⁴,
Nanna L. Meyer⁵, Arthur D. Stewart⁶, Wolfram Müller⁷

1. University of Western Australia, Perth, Australia
2. University of Arizona, Tucson, USA
3. The Norwegian School of Sport Sciences, Oslo, Norway
4. Loughborough University, Loughborough, UK
5. University of Colorado and United States Olympic Committee, Colorado Springs, USA
6. Robert Gordon University, Aberdeen, UK
7. Karl-Franzens University and Medical University of Graz, Austria

Corresponding author:
Winthrop Professor Tim Ackland
School of Sport Science, Exercise and Health
The University of Western Australia
M408, 35 Stirling Highway
Crawley, WA 6009
Australia
P: +61 8 6488 2668
F: +61 8 6488 1039
E: tim.ackland@uwa.edu.au

Running title: Body Composition Assessment in Sport

Key words: body composition methodology, bone density, dehydration, ultrasound, weight loss

Word count: 8220

TABLE OF CONTENTS

ABSTRACT

INTRODUCTION

Terminology

REVIEW OF TECHNIQUES

Reference methods

 Cadaver dissection

 Multi-component models

 Medical imaging – MRI and CT

Laboratory methods

 Dual energy x-ray absorptiometry (DXA)

 Densitometry

 Hydrometry (body water)

 Ultrasound

 3D photonic scanning

Field methods

 Anthropometry

 Bioelectrical impedance analysis (BIA)

 Body mass index (BMI) and mass index (MI)

SUMMARY AND CONCLUSION

FIGURE CAPTIONS

Figure 1. Chemical and anatomical body composition models. 4-C, 3-C and 2-C refer to four, three and two-component models respectively.

Figure 2. Comparison of subcutaneous adipose tissue (SAT) thickness measurements: 140 distances measured in swine carcass by means of ultrasound (d_{US} ; $f = 7.5$ MHz) compared to vernier calliper measurements (d_{VC} ; resolution: 0.01 mm). Correlation coefficient was 0.998 and regression coefficient was 0.98 using $c = 1540$ m/s and 1.00 for $c = 1510$ m/s. Data from Horn and Müller^[48].

Figure 3. Semi-automatic image evaluation: The edge detection algorithm for subcutaneous adipose tissue (SAT) thickness determination enables selecting areas of interest, distances (d_{US}) measurement series, color-coding of distance values, and statistical evaluations^[48]. In this example of a SAT-layer above the triceps muscle, with the transducer held parallel to the humerus, 119 d_{US} values ranging from 2.3 mm to 4.3 mm were automatically detected by the algorithm; the median was 3.4 mm ($c = 1470$ m/s). Layers and interfaces: A: gel, B: gel-epidermis, C: dermis, D: dermis-SAT, E: SAT, F: SAT-fascia of muscle, G: muscle.

Figure 4. A skinfold map illustrating extreme leanness in elite adult male (dark) and female (light) endurance athletes of similar skinfold total. Measurements in mm.

Figure 5. Average skinfold depth across seven or eight sites, according to athletic group. Upper chart: males; lower chart: females. Data calculated from summary presented in Kerr and Stewart^[77]. Abbreviations: mid dist = middle distance track runners; long dist = long distance runners; Scot long dist = Scottish long distance runners; SASI mid dist = South Australian Sports Institute middle distance track runners; SASI sprint = sprint runners; SASI jump = jumpers.

Figure 6. Selected skinfold ratios in extremely lean male and female endurance athletes, and mean values from 106 male and 33 female athletes^[80].

ABSTRACT

Quantifying human body composition has played an important role in monitoring all athlete performance and training regimens, but especially so in gravitational, weight class and aesthetic sports wherein the tissue composition of the body profoundly affects performance or adjudication. Over the past century, a myriad of techniques and equations have been proposed, but all have some inherent problems, whether in measurement methodology or in the assumptions they make. To date, there is no universally applicable criterion or “gold standard” methodology for body composition assessment. Having considered issues of accuracy, repeatability and utility, the multi-component model might be employed as a performance or selection criterion, provided the selected model accounts for variability in the density of FFM in its computation. However, when profiling change in interventions, single methods whose raw data are surrogates for body composition (with the notable exception of the BMI) remain useful.

ACKNOWLEDGEMENT

The authors wish to acknowledge the support from the Medical Commission of the International Olympic Committee in creating the Ad Hoc Research Working Group on Body Composition, Health and Performance. This review of the status of body composition assessment methods was one of the primary objectives of the working group.

INTRODUCTION

Body composition is an important health and performance variable. In weight-sensitive sports, many athletes use extreme methods to reduce mass rapidly or maintain a low body mass in order to gain a competitive advantage. As a consequence, athletes with very low body mass, extreme mass changes due to dehydration or eating disorders, extremely low percent body fat (% fat), or insufficient bone mineral density are becoming common issues in many sports^[1,2]. Deliberately induced underweight or short term mass reduction may lead to severe medical problems with sometimes fatal consequences^[1]. The weight-sensitive sports in which extreme dieting, low % body fat, frequent mass fluctuation and eating disorders have been reported, can be summarized in three groups:

- Gravitational sports – in which mass restricts performance due to mechanical (gravitational) reasons. Among these are long distance running, ski jumping, high jumping and road cycling.
- Weight class sports – in which unhealthy short term mass reduction behaviour, associated with extreme dehydration, can be observed because the athletes anticipate an advantage when they are classified in a lower weight category. This group includes the sports of wrestling, judo, boxing, taekwondo, weight lifting and lightweight rowing.
- Aesthetic sports – in which athletes or their coaches expect higher scores when their body mass and shape conform to a perceived body ideal. This group includes particularly the judged female sports of rhythmic and artistic gymnastics, figure skating, diving and synchronized swimming.

Body fat may act as ballast in biomechanical terms, but adipose tissue is a vital endocrine organ in terms of general health. The different biomechanical and health imperatives present a conflict for athletes, for whom risks of eating disorders are exacerbated. To our knowledge, few of the international sport federations have considered implementation of programs aimed to discourage athletes from extreme dieting or from rapid mass loss by means of dehydration. The International Ski Federation (FIS) has changed regulations^[3,4,5] in order to improve the low mass problem, but more can be achieved in this area. An important step on the path toward maintaining an athlete's health and performance, by means of rule changes, is the ability to assess the athlete's body composition with accuracy, precision and reliability.

Understanding and quantifying human body composition has formed a central part of medical research for the best part of a century. While progress has been significant with landmark studies and the use of new and combined analytical methods, unassailable ethical and methodological limitations have precluded the identification of an absolute standard against which methods can be compared in humans. As a consequence, while accurate assessment of body fatness has been a major goal of body composition research over the past 50 years, much of the work to validate new and old methods is

indirect. Despite considerable advances in methods, today there is still no gold standard for body fat assessment with accuracy better than 1%.

Quantification of fat has been the prime focus of attention, but many coaches and scientists working with elite athletes recognize that knowledge of the amount and distribution of lean tissues like bone and muscle can be just as important in determining sports performance. For example, the relationship between muscle cross-sectional area and force/power generation is well known and so change in muscle size (relative to body mass) becomes an important assessment parameter during preparation for high level competition. Making sense of the myriad of techniques for estimating each of the tissue components requires a clear framework by which these may be properly compared.

During the development and integration of such multi-component methods, the last three decades have also been witness to a dramatic increase in research on elite athletes from a whole range of sports. As training methods have become more sophisticated, each athletic group has become more specialized, modifying its typical physique imperatives away from general morphological norms. As a consequence, many of the assumptions on which some techniques rely are no longer valid for athletes. For example, elite athletes who had undergone resistance training were estimated to have negative 12% fat using densitometry^[6] and to have negative fat on the torso using DXA^[7]. Furthermore, athletes are reluctant to interrupt what for many is a full time occupation for the sake of body composition assessment, thereby making the more involved laboratory techniques less appealing. These factors all conspire against the scientist seeking to make accurate measurements on athletes, with the inevitable consequence that data may be misleading, misinterpreted, or perhaps used inappropriately. This reality has forced researchers to consider acceptable surrogate measures for fatness, such as a sum of skinfolds, without recourse to quantifying tissue mass.

The choice of body composition technique often depends on the intended purpose for which data are to be used, as well as the available technology. In regard to high performance sport, assessment of body composition may define a performance or selection criterion, be used to assess the effectiveness of an exercise or dietary intervention, or be used to monitor the health status of an athlete. Individual body composition goals should be identified by trained health care personnel (e.g. athletic trainer, physiologist, nutritionist, or physician) and body composition data should be treated in the same manner as other personal and confidential medical information.

In addition to the published journal articles, books and book chapters written by the authors of this review, several online databases (including Medline and Sports Discus) were searched to provide the most current publications to inform this review paper.

REVIEW OF TECHNIQUES

Though many techniques exist for describing the constituent components of the body, in practice the techniques in current use fall into Reference, Laboratory and Field method categories, which include both the Chemical (Molecular) or Anatomical (Tissue/Systems) approaches (Figure 1). Within these approaches, we must also understand that techniques can be categorized as being Direct – for example via cadaver dissection, Indirect – where a surrogate parameter is measured to estimate tissue or molecular composition, or Doubly Indirect – where one indirect measure is used to predict another indirect measure (i.e. via regression equations). The use of regression equations also means that these approaches are sample-specific. Hawes and Martin ^[8] refer to these categories as levels of validation.

Insert Figure 1 near here

In both the Chemical and Anatomical approaches, we may also employ multi-component models (Figure 1). Thus, it has been common for authors to refer to 2-component models (fat mass [FM] and fat free mass [FFM]), 3-component models (fat, bone mineral and lean content), or 4-component models (adipose, bone, muscle and other tissues).

A review of body composition methods must also consider the implications of techniques that merely sample the body as opposed to those which attempt to assess the whole body. Several commonly employed methods (e.g. skinfolds, ultrasound) sample the subcutaneous adipose tissue (SAT) at standardized sites and assume that there is some fixed and direct relationship between this compartment and fat depots deep within the body. Furthermore, it is assumed in these methods, that the standardized sites provide a representative estimate of the total subcutaneous fat in the body.

Finally, mention must be made regarding individual versus group results. Some techniques that supposedly assess body composition (e.g. body mass index [BMI]) are often cited as being significantly correlated with important health indicators, or values from other assessment procedures. Readers are cautioned to understand that demonstration of a strong association at the population level is not the same as a technique providing accurate, precise and reliable body composition data for an individual.

Reference methods

The reference methods are, by definition, the most accurate techniques for assessing body composition and have often been employed as criterion against which other techniques are compared. Nevertheless, these reference methods may have limited applicability for monitoring athletes. Limitations include feasibility (eg. cadaver dissection), time and financial costs involved (eg. MRI scanning), a lack of published normative data (e.g. multi-component models), and unnecessary radiation exposure (eg. CT scanning). There are also questions regarding sensitivity (acuteness) of some of the accepted reference methods. A summary of the important features of these techniques is provided in Table I.

Insert Table I near here

Cadaver dissection

Human body composition analysis is unique in that validated measures can be ascertained only via cadaver dissection. Even so, this approach does have several limitations (Table I). Aside from the use of porcine carcasses to validate DXA, time, cost and for cadavers, inescapable ethical barriers, limit the use of this technique. Results from the Brussels Cadaver Study were employed to test several assumptions related to the anthropometry field method of body composition analysis^[9,10,11]. Since the cadaver dissection method cannot be utilized for individual analysis, practitioners have turned to other reference, laboratory and field methods for estimating body composition.

Multi-component models

The best reference methods for estimation of body fat are the multi-component models. Both their precision and accuracy are in the order of 1-2%. Elaborate 6-, 5-, 4- and 3-component models are available for body fat estimation^[12]. The 4-component model using body density, body water and bone mineral is the most often used method and is, at present, the leading reference method for body composition. Wang et al.,^[12] presented 13 different 4-component equations, each with different assumptions for the various components. The 4-component equation is always in the form of:

$$\text{Fat Mass} = C_1 \text{BV} - C_2 \text{TBW} + C_3 \text{M} - C_4 \text{BM}$$

Where: BV is body volume, TBW is total body water, M is bone mineral and BM is body mass.

The most practical multi-component model measures body density and body water and can estimate fatness within standard errors of estimate (SEEs) of 2.0-2.5% (3-component model). Precision of multi-component models is high^[12,13,14]. Technical errors of estimating body volume, body water and bone mineral have been combined to yield a % fat error of about 1%. Accuracy is in the order of 2%

^[15], and even better when a 5-component model is used ^[12]. However, when body water estimations are not accurately assessed, as in the case of Clasey et al., ^[16], then larger errors in the multi-component models are apparent. Compared to the data by Wang et al., ^[17] for example, the variation (SD^2) between water variability (variance) is 3.2 times greater in the Clasey et al., ^[16] sample. This variability exceeds the biological variation in water/FFM content under usual hydration conditions, thereby signifying a large technical contribution. Multi-component assessment models are time consuming and require access to expensive and sophisticated technology which often places them out of reach for practical applications in sport.

Medical imaging – MRI and CT

MRI is a highly sophisticated and costly technique which has become the premier medical imaging technique during recent years. It requires a powerful main (usually superconducting) magnet, a magnetic field gradient system, which is essential for signal localization, and a radio frequency system, which is used for signal generation and processing. Like other tomographic imaging techniques, MRI scanning results in a data array (MRI image) which represents the spatial distribution of some measured physical quantity. The values of the image pixels depend on various parameters of the tissue under study: MRI produces images of internal physical and chemical characteristics of an object from externally measured nuclear magnetic resonance (NMR) signals. The effects of these tissue characteristics on the NMR signal can be enhanced or suppressed by using appropriate data acquisition protocols. MRI's flexibility in data acquisition can result in quite different images for the same anatomical region, depending on the parameter setting. The soft tissue contrast, which depends largely on the design of the pulsing sequence, exceeds that of CT and of US. No ionizing radiation is involved, so the method is not invasive, although the confined space of the scanner may induce claustrophobia. It is beyond the scope of this review to describe MRI in detail, and readers are referred to Runge et al. ^[18] or Liang and Lauterbur ^[19] for further information.

Despite its sophistication, this technique requires powerful software for analysis involving setting thresholds for different tissues. Most software in clinical use is designed for diagnostic purposes, not for quantifying tissue dimensions beyond the organ level. Whole body scans are possible, but need to be acquired as a series of stacks and subsequently integrated. Currently, the pixel size of 2 mm x 2 mm in slices used in total body scans limits the accuracy of measurement, particularly in lean athletes. Difficulties in discriminating boundaries between tissue layers further limits sensitivity.

CT is also capable of high resolution internal images of the body, but involves a high radiation dose because its image acquisition is based on X-rays which are configured in a perpendicular plane to the supine participant. The X-ray tube and detector follow a rotational path-enabling image

reconstruction following the measured attenuation relative to air and water, quantified in Hounsfield units. Tissues vary in their radiographic density; skeletal muscle has a much higher range than adipose tissue, enabling easy distinction and quantification of each. However, whole body scanning in living humans is not feasible due to an unjustifiably high radiation dose, and most studies rely on interpolation between slices of measured composition. Both MRI and CT produce tissue distances, areas and volumes which, if related to multi-component models of body composition, require assumptions to relate to mass via assumed density and/or chemical composition. As a consequence of the several limitations associated with MRI and CT, neither represents a practical method for everyday body composition assessment.

Laboratory methods

The laboratory methods are used extensively for assessing body composition of athletes (though perhaps not to the same degree as field methods), but there exists wide variation in their accuracy and precision. A summary of the important features of these techniques is provided in Table II.

Insert Table II near here

Dual energy x-ray absorptiometry (DXA)

For over two decades, DXA has been the diagnostic method of choice for osteoporosis and has been used increasingly in the quantification of soft tissue. It achieves this by passing filtered X-ray beams at two different photon energies through the participant which are attenuated differentially by the material in their path. With the participant lying on the scanning table, the process maps the mass and composition of each pixel in terms of bone mineral, fat and fat-free soft tissue. FM is determined by the ratio of soft tissue attenuation at the two energies, and *in-vivo* elemental composition supports the underlying physical concept of this being accurate ^[17]. DXA has been criticized because it assumes segment constancy in tissue composition; however, both water and lipid content of skin, adipose, muscle and bone tissue exhibit regional variation ^[20]. Despite a low radiation dose (which varies according to the scanner type and beam configuration, and consequentially requires a pregnancy test in women of child-bearing age), this method is viewed as a laboratory reference method and contributes to the bone mineral assessment for multi-component models. DXA's utility and widespread proliferation in current practice has rested on the convenience of acquiring regional composition data without recourse to the more costly and scarce medical imaging techniques. However, we must caution against using DXA on multiple occasions (perhaps no more than four times per annum), not only due to the cumulative radiation dose (including all other sources from medical imaging), but also due to the error of measurement which limits the ability to detect small

composition changes over time. Although effective doses associated with DXA measurements are low when compared to X-ray imaging, we do not encourage frequent or indiscriminate DXA testing.

Multi-component models as a reference method to validate DXA are now extensive^[15] with SEE for predicting % fat falling between 2-3%, representing a major advance in laboratory and clinical practice for estimating body composition. The theoretical basis and the assumptions DXA makes in deriving composition estimates are discussed in detail in the review of Pietrobelli and colleagues^[21]. These relate to beam hardening (due to the depth of tissue encountered by the X-ray beam) and errors of estimating fat quantity in the approximately 40% of scan pixels which contain bone (estimated by the measured composition of neighbouring pixels with no bone). With the more recent fan-beam scanners, magnification errors may also limit accuracy in larger subjects.

For athletes, DXA measurement has several advantages over other reference and laboratory techniques, due to its speed and convenience, and because the measurement is minimally influenced by water fluctuation. However, measurement of athletes who are excessively small, large or lean may introduce errors greater than for subjects of standard size and composition. Individuals greater than ~192 cm may be too tall for the scan bed, while the soft tissue of very obese people may migrate beyond the available width of the scan area. The more recent scanners can accommodate individuals of 120 kg, but strength athletes may exceed the mass permitted by older models.

DXA has been used to derive regional and total fat estimates which outperformed densitometry relative to a 4-component model^[22]. This led some authors to use it as a reference method in preference to densitometry, yielding FM and FFM predictions from other methods. In a study of male athletes, SEE predicting DXA-derived FM from skinfolds was 1.7 kg, although the seven leanest athletes showed negative fat on the torso^[7]. The high muscle mass and low FM of these individuals appear to fall beyond the calibrated range. Of some considerable concern then, is the ever-increasing access to DXA by commercial sports organisations that seek to measure incrementally lean and muscular individuals, meaning the scope for misinterpretation of data is also increasing.

DXA has been compared with CT and neutron activation analysis for assessing skeletal muscle mass with SEE of 1.6 kg and 4.4 kg respectively^[23]. Further validation studies by Wang et al.,^[24] and Kim et al.,^[25] concluded that skeletal muscle mass could be accurately predicted by DXA. However, Tothill et al.,^[26] showed considerable regional differences between machine manufacturers and pencil versus fan beam configurations for estimating fat and bone mineral. While apparent bilateral composition differences are likely to result from positioning and regional division lines falling at pixel boundaries, observed variations in fat estimation also relate to different assumptions of the fat

distribution model used in the software. Further, some fan beam scanners have significantly overestimated the leg muscle mass derived by CT in elderly individuals ^[27], and the effect is likely to be exacerbated amongst athletes.

In summary, DXA, though a reasonably precise whole-body method, is not reliable in producing accurate fat estimates of lean athletes, although its assessment of total and regional FFM is generally acceptable if total scanned mass equates to scale mass. Inter-manufacturer differences in hardware and software algorithms preclude straightforward or meaningful comparisons between apparatus.

Densitometry

Body density measurements, using either underwater weighing (UWW) or air displacement plethysmography (ADP) to estimate % fat, are based on the 2-component model. This divides the body into FM and FFM, assumes a constant density of each, then relates the measured whole body density to a % body fat ^[28,29]. Lipid is the only constituent of the body whose specific gravity is less than that of water (1.0) and its buoyant force is opposed by all other, denser constituents. Variations in water and bone mineral content of the FFM among populations and individuals affect its density and therefore, limit the utility of this approach as a reference method ^[30].

UWW requires a participant (on a submersible seat suspended from a load cell) to exhale maximally during submersion. Calculating body density relies on dividing body mass by the measured volume. Although less subject involvement is required using plethysmography, both methods require estimation of residual lung volume with additional equipment and expertise. In UWW, this is routinely performed using oxygen dilution ^[31] and should be done in the water because hydrostatic pressure affects measured lung volumes.

ADP follows a similar approach by measuring body volume, but in a sealed air capsule, rather than under water. By comparison, ADP is rapid, does not require water confidence, and is suitable for a wider range of individuals. Currently, the available ADP technology is referred to as the BodPod (Life Measurement Inc., Concord, California, USA). In this system a measuring chamber and a reference chamber (beneath the seat) are linked by a flexible airtight diaphragm which is perturbed to induce small pressure changes between both chambers. Using Poisson's Law, the pressure-volume relationship at a fixed temperature is used to calculate the volume of the participant in the measuring chamber. After the system has been calibrated with a known volume, the participant is weighed wearing swimwear and cap, then occupies the measuring chamber for ~2 min for volumetric measurement. Breathing normally during measurement, the participant is then prompted to execute a breathing manoeuvre for residual gas calculation. Adjustments for thoracic gas volume and skin surface area are necessary because of the behaviour of the air inside the chamber.

Despite its advantages over UWW in participant acceptability and throughput, several methodological issues require consideration. Moisture on the skin or hair affects compressibility of air next to the body surface, leading to an underestimation of % body fat. The behaviour of air close to the skin surface is predicted by a surface area artefact, based on estimated body surface area. Such estimates may under- or over-estimate an athlete's true surface area. Clothing is also important with swimwear recommended; wearing gym apparel reduces test-retest reliability and leads to an underestimate of fatness^[32]. Peeters and Claessens^[33] also demonstrated that a lycra cap compresses the hair less effectively than a silicon cap, not fully eliminating the effect of isothermal air trapped in scalp hair, which also results in an underestimation of fatness. While such issues of participant presentation are easily addressed, more problematic may be locating the capsule, which requires a separate room, with closely regulated temperature and humidity. Changes in ambient pressure through windows or doors may cause the system to require re-calibration.

Variations in % body fat have been reported for gender between UWW and ADP^[34]. Compared with results from UWW, ADP underestimated % body fat (in absolute terms) by 8% in lean female athletes^[35], underestimated % body fat at lower fat values and overestimated at the higher fat values in boys^[36], and under-predicted % body fat by an average 2% in male college football players^[37]. In summary, despite the popularity of densitometry techniques over many decades, both UWW and ADP techniques adopt the 2-component model that assumes density of FFM to be constant. This assumption is clearly violated in many groups of athletes. Therefore, caution is essential when interpreting body fat results from these methods, especially for lean athletes.

Hydrometry (body water)

Except in the very obese, water is the largest single component of the body, typically accounting for 50-70% of total mass. The water content of different tissues varies, but lean tissue is generally 70-80% water, while adipose tissue is generally about 20% water^[38]. There is, however, not agreement on this and the Institute of Medicine^[39] used a value of 10% for the water content of adipose tissue.

Total body water can be used to estimate both FM and FFM assuming a constant hydration of 72-73%. Variation in hydration levels among subjects is the main limitation of this method for the athletic population. Body water can be used to estimate fatness within 3% and when combined with body density, to within 2%. The primary approach for body water measurement is the deuterium dilution method, which was well described by Schoeller et al.,^[40]. However, body water assessment relies on purchase of deuterium oxide (a stable isotope), expert measurement skills and expensive laboratory equipment, so is not generally available for wide-spread body composition assessments.

An understanding of hydration status has implications for all body composition assessment techniques. Although the rate of turnover of body water is typically about 2-3 L/day, it can be much higher than this, with losses through faeces reaching 1 L/h during acute infectious diarrhoea and sweat losses in excess of 3 L/h being sustained for relatively short periods during physical activity in hot environments. Daily fractional turnover can, therefore, reach 30-50% of total body water. Acute changes in body water can confound the use of standard methodologies for the assessment of body composition. For a 70 kg individual with 14 kg of fat (20%), a loss of 10% of body water will increase the fraction of fat to 21.5%. All measures of body composition should, therefore, be made under standardized conditions of hydration status (e.g. after fasting, prior to an exercise bout, with an empty bladder). Euhydration, however, is difficult to define as it is a dynamic state.

The literature indicates that a number of methods have been used to determine hydration status. Body mass changes, urinary indices (volume, colour, protein content, specific gravity and osmolarity), blood borne indices (haemoglobin concentration, haematocrit, plasma osmolarity and sodium concentration, plasma testosterone, adrenaline, noradrenaline, cortisol and atrial natriuretic), bioelectrical impedance analysis (BIA), and pulse rate and systolic blood pressure response to postural change are discussed. The urinary measures of colour, specific gravity and osmolarity may be more sensitive at indicating moderate levels of hypohydration than are blood measures of haematocrit and serum osmolarity and sodium concentration.

All methods, however, are subject to errors as a result of recent fluid intake; acute ingestion of a bolus of water can produce relatively dilute urine even in a hypohydrated individual. Currently, no 'gold standard' hydration status marker exists, particularly for the relatively modest levels of hypohydration that frequently occur during exercise. The choice of marker for any particular situation will be influenced by the sensitivity and accuracy with which hydration status needs to be established, together with the technical and time requirements, and the expense involved.

Ultrasound (US)

Ultrasound imaging is based on the pulse-echo technique. A short US pulse is applied and travels with the speed of sound (c) in the given tissue. Most diagnostic US machines use $c = 1540$ m/s for calculating the distance from the source to the boundary between two tissues having different acoustic impedances: $d = c T/2$ (T is the echo time). For 2D imaging US beams are sent sequentially into the tissue for creating an image in which the brightness of the screen (B-mode) corresponds to the echo intensity in the plane of the scan. Diffraction limits spatial resolution approximately to the wavelength used. Frequencies between 3-22 MHz are generally employed, corresponding to wavelengths in soft

tissue of 0.5-0.07 mm. Maximum resolution is limited because attenuation of sound increases with higher frequency.

High accuracy of US fat thickness measurements in humans was described in 1965^[41] and 1966^[42] and many studies then followed^[43]. The precision of SAT measurements was found to be excellent (technical error in both intra- and inter-observer studies was less than 0.15 mm at all sites investigated except for triceps [0.6 mm])^[44]. Ishida et al.,^[45] found B-mode US to be a highly reliable method for measurement of both fat and muscle thickness. US imaging has also been suggested for visceral fat mass evaluation^[46]. An US approach for precise and accurate measurement of skin thickness has recently been described by Moore et al.,^[47]. Considerable skill and anatomical knowledge may be needed to identify correctly the interfaces of the tissues of interest. For SAT thickness measurements, however, the adipose tissue layer is comparatively easy to find as it forms a continuous layer underneath the skin which is bounded by the muscle fascia at the deep edge.

Recently, Horn and Müller^[48] compared US ($f = 7.5$ MHz) SAT measurements in excised pig tissue using a semi-automatic image evaluation procedure with vernier caliper measurements (0.01 mm resolution); the correlation was very high ($r = 0.998$; $n = 140$) (Figure 2) and SEE was 0.21 mm. The regression coefficient was 0.98 when (standard) sound velocity of 1540 m/s was used and 1.00 was obtained for 1510 m/s, indicating a lower speed of sound in fat. However, thickness measurement error due to sound speed deviation is small (e.g. 3% for a speed deviation of 50 m/s).

Insert Figure 2 near here

In this technique, it is important for the investigator to control visually the output of automatic edge detection algorithms so as to prevent erroneous image interpretations. An example for SAT measurements using recently developed semi-automatic evaluation software^[48] is shown in Figure 3.

Insert Figure 3 near here

Many thickness measurements can be obtained from a single US image, resulting in a very low standard error of the mean (SEM). Accuracy demands beyond the capability of US are of little relevance because of accuracy limitations due to the tissue's plasticity.

It is another advantage of US that many measurements can easily be made in the vicinity of a given site where thickness varies greatly and mean values can be used instead of single point measurements. US is well suited to analyse fat patterning and total SAT may be determined by combining a series of US measurements with body surface area measurement techniques like laser scanning. It should be

expected that estimates of total body fat or total subcutaneous FM based on US method will result in higher accuracies when compared to skinfolds, BIA, and backscattered light techniques. However, appropriate protocols for estimates based on US have not yet been standardized.

Due to the high accuracy of SAT measurements at given sites, US can be used to calibrate other imaging techniques like MRI or CT. It could be used for optimizing the image segmentation protocol, which is always a crucial problem in MRI and CT image analysis. Pixel size in MRI whole body scans is typically 2 by 2 mm and SAT thickness can be below 1 mm in lean athletes - therefore high errors at certain sites are to be expected for such scans. A literature survey on accuracy of MRI is given by Ross and Janssen^[49] and comparative studies of MRI and US for visceral and subcutaneous fat evaluation were published by Koda et al.^[50].

In summary, it can be expected that US thickness measurements in adipose, muscle and other tissues will gain a leading role because of the high measurement accuracy. Future studies are needed, though, to establish standard measurement sites and protocols. Small, transportable US machines are also available which will enable application in the field.

3D photonic scanning

3D photonic scanning enables profiling of the body in unprecedented ways. Its development over the past 25 years for the clothing and automotive industries has included approaches using structured light, class 1 (eye-safe) lasers or millimetre wave technologies. These have made contributions to epidemiological research and, more recently, sport science.

Photonic scanning data have shown men and women to be fundamentally distinct in BMI-shape relationships^[51], have quantified the effect of age in varying shape at a given body size^[52] and have explored the contrasting shapes of those of different ethnicity, at a similar level of BMI^[53]. 3D scanning has also been validated for assessing body volume and subsequent % fat prediction following appropriate accounting for lung volumes^[54]. However, application of such a protocol requires subjects to breathe out fully whilst being scanned, which might be limiting for some individuals as it is for UWW. A study of military personnel found good agreement between % fat derived from 3D scanning (Cyberware) with in-house software and DXA (GE Lunar Prodigy)^[55], although the strategy for assessing the lung volume to subtract from scan volume before calculation of % fat was not stated. In this respect, 3D and DXA scanning share the commonality of 'undisclosed algorithms' for arriving at fatness and thereby, unquantified error, which future research must address.

The requirement for participants to wear form-fitting clothing, which can be a severe limitation in obesity or body image research, is no impediment for research with athletes, many of whom are

required to wear such clothing in training and competition. To date, no study assessing body fatness in athletes via 3D scanning has been undertaken because of the limited availability of scanning facilities. However, recent access to this technology by elite athletes has enabled quantification of body segments amongst rowers, yielding data (such as segmental volumes) which quantify variability and effect sizes relative to controls from the general population ^[56]. These findings are clearly significant for talent identification and could not have been assessed using conventional anthropometry.

In summary, this novel approach does not attempt to quantify minimum weight or fatness, but is a potentially useful adjunct to existing measures, which may be pertinent in weight-restricted sports. Alone, the method measures body volume with some accuracy, but incorporates the same assumptions and limitations as densitometry when estimating FM and FFM. Nevertheless, the rapid profiling enables great numbers of athletes to be surveyed within the limitations of time and cost. Finally, its combination with other measurement modalities such as US and DXA will undoubtedly represent a major advance in future body composition research.

Field methods

Field methods are most often employed for monitoring body composition in both sports and health applications, but with varying degrees of validity. A summary of the important features of these techniques is provided in Table III.

Insert Table III near here

Anthropometry

The acquisition of surface dimensional measurements as surrogates of composition was pioneered by Jindrich Matiegka ^[57] and subsequently applied to Olympic athletes at the 1928 Amsterdam games and thereafter, notably at the 1960 Rome games to characterize somatotype, proportions and size variability among sports ^[58]. To date, well over 100 body fat prediction equations have been developed from skinfold measurements ^[59] and their inconsistent outcomes result from the differences in populations sampled, and lack of rigour in standardizing the technique. For instance, varying the skinfold site by as little as 1 cm produces significantly different results when experienced practitioners measure the same participant ^[60]. Precise definitions for measurement sites, in addition to a standardized technique are, therefore, of fundamental importance for this method.

To this end, 1986 saw a national standardization conference in Airlie, Virginia (USA) which resulted in a manual ^[59]. Simultaneously in Glasgow (UK), the International Society for the Advancement of

Kinanthropometry (ISAK) was formed, which subsequently established an exam-based certification scheme for practitioners and instructors, and a closely-defined protocol ^[61]. Both manuals represent significant progress in the quality of data derived from anthropometric measures, usually quantified by statistics of replicate measures. ISAK instructional courses often result in a seven-fold reduction in intra-tester error. However, high precision with a single measurer can mask systematic differences between measurers and crucially, only under the ISAK scheme is inter-tester error also quantified.

Fatness has been predicted from skinfolds, circumferences and skeletal width, usually validated against densitometry. In some cases SEE of the skinfold method was estimated to be less than 3% when variation in the reference method was taken into account, though in generalized equations ^[62] this value approached 5%, which is an unacceptably large error. While many generalized equations have been cross-validated for specific samples, their use in determining fatness in athletes relies on conforming to the assumptions both of anthropometry and densitometry. Out of 18 such equations only three were found to be reliable for use in athletes ^[63].

A cross-validated skinfold equation for USA high school wrestlers was produced in order to standardize the approach to establishing minimum weight. Produced on 860 wrestlers across five universities, the study tested the validity of 16 equations, the best of which estimated the densitometry-derived minimum weight with an SEE of 2.4 kg based on the sum of three skinfolds ^[64]. The results indicate that the equations developed by Lohman ^[65] with three skinfolds, Thorland with seven skinfolds and Behnke ^[66] with a combination of skinfolds, circumferences and skeletal widths, all predicted minimum weight with a total error of 2.5 kg. This approach involved young adult wrestlers, but could be generalized to other athletic groups, if a large validation study were performed. However, such a study would need to ensure that the reference method was obtained via a multi-component model, because of the known violation of the assumed density of the FFM using densitometry alone.

While circumferences can estimate body fatness (SEE > 3%), they represent variability in frame size and muscularity in addition to fat. However, combining skinfolds and circumferences does not increase the prediction of body fat over skinfolds alone ^[64]. Similarly, the use of skeletal breadths to estimate body fatness has an SEE > 4% and offers no improvement over skinfolds in assessing either fatness or estimating minimal weight. Another approach which has been widely reported in the obesity literature is the use of anterior-posterior abdominal thickness or ‘sagittal abdominal diameter’. This dimension has been particularly associated with identifying visceral fat accumulation ^[67], metabolic syndrome ^[68], cardiovascular risk ^[69] and shape change during weight loss ^[70]. While this might not initially seem a strong candidate for use in athletes, it is possible that abdominal dimensions could provide a framework for a normal anticipated shape once normative data have been established.

An alternative to converting skinfolds to body fat and minimum weight is the approach promoted by Marfell-Jones ^[71] who highlighted the value of using skinfolds as a valid proxy for adiposity. Individual and sum of skinfolds can be compared to published norms for Olympic or world class athletes ^[72,73,74,75,76]. The rationale for proposing the skinfold thickness as a valid measure in its own right without conversion to FM or % body fat, centres on the avoidance of a series of assumptions which are known to be invalid – especially so in an athletic sample. These include assumptions of constant skin (dermis and epidermis) thickness, uniform subcutaneous adipose tissue compressibility, constant relative adipose tissue distribution, constant fat-fraction of adipose tissue, constant internal to external distribution of fat and above all, the assumed constancy of the FFM density. The resulting error in accurately estimating % body fat necessarily includes the additional errors of the reference method (usually densitometry), which have been identified to be greater amongst athletic groups.

Various regimens have summed values from different measurement sites in an attempt to capture a representative surface adiposity. While it is clear that certain sites such as the thigh and the iliac crest tend to be larger than others, such a pattern may alter with increasing leanness. This introduces a further level of complexity (explaining why generalized formulae may not be valid for athletes) and affords the opportunity to track skinfold patterns, means or ratios with leanness. The first of these is best depicted in a radial plot known as the skinfold map (Figure 4) where the profile can be used for tracking individual change or comparing an individual to group data.

Insert Figure 4 near here

Using the data presented by Kerr and Stewart ^[77], the average skinfold magnitude across sites assessed by ISAK-qualified practitioners varies considerably by sport and is generally lower in males than females as depicted in Figure 5.

Insert Figure 5 near here

Using the same approach and comparing these grouped athlete profiles with those of a cohort of adult anorexic patients ^[78], we discover that female gymnasts have lower, but all other female athletes slightly higher, scores. It is important to recognize the probability of individuals displaying different thresholds of minimum skinfolds before health or performance deteriorate – so applying group data to individuals requires caution.

As is the case for extreme obesity, in extreme leanness, the sexual dimorphism becomes less apparent – in other words, the characteristic fat patterning associated with males and females becomes less

distinct with reduced variability in skinfold magnitude across sites. Nevertheless, some distinctiveness remains, with the male profile having the highest value at the subscapular site, while the female profile is highest at the thigh. This can be seen in greater detail by considering skinfold ratios. These have been used extensively in tracking fat patterning during childhood growth, but may have a role in identifying minimum fatness in athletes. Figure 6 depicts the leanest of an athletic sample for selected skinfold ratios (the same individuals as in Figure 4) and also the equivalent mean values for 106 male and 33 female elite athletes from a range of sports ^[79].

Insert Figure 6 near here

A number of interesting observations can be made from Figure 6, including that subscapular:triceps, thigh:abdominal and triceps:biceps skinfold ratios all appear to exhibit a difference between the leanest and mean values, thereby suggestive of a 'physique gradient' of fat patterning. On the contrary, the abdominal:medial calf ratio displays no such gradient, although gender differences appear preserved. The abdominal:iliac crest ratio appears to depict neither a physique gradient, nor sexual dimorphism. While caution may be advised in the use of ratios as opposed to absolute values as a result of error propagation, ratios appear ubiquitously throughout exercise science for monitoring athletes, and a combination of absolute and ratio scores (in conjunction with health and performance measures), might best serve scientists seeking to use skinfolds to establish a system of flagging inappropriately low body fat levels and alerting athletes, coaches and medical staff accordingly.

In summary, anthropometry provides a simple and highly portable field method for estimating body composition via surrogate measures for fatness and muscularity. Provided the measurer is well trained and follows a standard protocol, the assumptions of the technique are acknowledged, and the data treatments are not confounded with additional sources of error (conversion to %FM/FFM), anthropometric techniques have widespread utility for monitoring athlete body composition.

Bioelectrical impedance analysis (BIA)

The total volume of a conductor can be estimated from its length (L) and the resistance (R) to a single frequency electric current (L^2/R). This principle has been applied to body composition assessment using BIA. The key assumptions are that the conductor is cylindrical in shape and that the current is distributed throughout the conductor uniformly ^[81].

Multifrequency bioimpedance can be used to quantify distribution of extra- and intra-cellular water with important applications to the medical field in the areas of fluid balance and monitoring various patient groups including hemodialysis and other renal disease patients ^[82]. The work of Wabel et al., ^[83] indicates the extensive use of BIA spectroscopy in the management of fluid balance to prevent

both fluid overload and dehydration. Applications to the dehydrated athletic population have yet to be developed.

Though BIA has been used widely to estimate body composition, and many equations have been reviewed ^[81], its accuracy is limited in estimating body water and body fatness. In a careful comparison between BIA and skinfolds among wrestlers, where several laboratories followed diligently the same measurement protocol, both methods predicted percent body fat (from densitometry) with an SEE of 3.5% ^[84]. This indicates clearly the accuracy limits with these measurement techniques, and the SEE values are obtainable only ‘within’ specific groups, but not for mixed groups of athletes. When individual body composition of an athlete is to be assessed, one should consider that, for example, 3% deviation from an assumed true value of 8% would result in % body fat values between 5-11%. This is far from the accuracy necessary for proper interpretation of health and performance optimization. While other studies using anthropometry have lower errors than this, a further limitation of the BIA method for athletes lies in the measurement pre-requisites which include abstaining from exercise.

Body mass index (BMI) and mass index (MI)

Several indices expressing mass relative to some power function of height have been suggested and tested for maximum correlation with mass and minimum correlation with height ^[85,86,87]. One that is widely used is the BMI (Quetelet's index) which relates body mass (m ; in kg) and height (h ; in m): $BMI = m/h^2$. Anthropometric values of height, body mass and sitting height can easily be measured with high accuracy, but these indices measure ponderosity, not fatness. Interpretation of mass with respect to stature (‘relative body mass’) is not a simple task. The WHO Expert Committee on Physical Status ^[88] stated: *“Problems arise, however, in adults whose shape differ from the norm ... Care should therefore be taken in groups and individuals with unusual leg length to avoid classifying them inappropriately as thin or overweight.”*

Therefore, leg length or sitting height (as an indirect measure for leg length) should also be measured when ponderosity is to be assessed. A recently introduced extension of the BMI formula termed mass index (MI) ^[3,4,5] has the advantage of considering the individual’s sitting height. In the general MI formula, the stature (h), sitting height (s), and body mass (m) determine the value of this index for ‘relative body mass, with C being the individual Cormic Index ($C = s/h$):

$$MI_k = BMI \left(\frac{\bar{C}}{C} \right)^k = \frac{m}{h^2} \left(\frac{\bar{C}}{s/h} \right)^k = \frac{m}{h^{2-k} s^k} \bar{C}^k$$

The value of 0.53 for \bar{C} , which is a value in the middle of the Cormic index continuum, represents ‘mean sitting height’. The exponent k weights the impact of the Cormic index. The unit of MI is

kgm^{-2} , as for the BMI, which is just the special case for k set to zero; in this specific case we get: $\text{BMI} = \text{MI}_0$ (no consideration of individual leg length). For $k=2$, the general equation reduces to ($\text{MI}_2 = 0.53^2 \text{ m/s}^2$) in which body height (h) does not appear. The choice of $k=2$ is in accordance with anthropometric data published by Norgan^[89] when a measure which is independent of C (and thus independent of leg length) is desired. However, the slope of the regression line in Norgan's publication is based on group mean values for BMI and C , which is not necessarily equal to the mean of the slopes of regression lines within individual groups. For $k=1$ we get ($\text{MI}_1 = 0.53 \text{ m/hs}$). Non-integer values for k can also be used. Further studies are necessary to identify the best value of k for appropriate consideration of individual leg length.

It has to be pointed out that no weight-corrected-for-body-dimension index can distinguish between fat and muscle mass of an individual. This inability of BMI to assess fatness or adiposity has been reported in the literature^[90]. Despite this limitation, the use of MI instead of BMI may permit diagnosis of underweight and assessment of 'optimum body weight' for high performance in sports on a finer scale. Sitting height or leg length is as easy to measure as stature^[91] and should be included in all basic data sets of athletes and patients. In young athletes, this will also assist in understanding problems associated with individual growth.

SUMMARY AND CONCLUSION

In summary, all of the techniques in common use have some inherent problems, whether in methodology, interpreting the data, or in the assumptions they make. Limitations in both the 2-component model (accuracy) and multi-component model (practicality) highlight the desire for an economical laboratory or field approach to body composition assessment that is both accurate and objective. In the absence of such a criterion technique, there is scope for several of the reviewed methods to play a useful role under certain circumstances. For example, where the body composition assessment is used as a performance or selection criterion, then technique accuracy and reliability are of paramount importance. The multi-component model might be employed here provided the selected model accounts for the variability of the density of FFM in its computation. In this case, health care and high-performance support staff must give due consideration to the technical error of measurement, and not apply an absolute criterion or threshold value for selection unilaterally. This is of particular importance when extremely lean athletes are examined.

However, if the athlete's body composition is being monitored to assess the effectiveness of an exercise or dietary intervention, the use of some laboratory or field method may be more practical.

Depending on the availability of technology and operator training, laboratory techniques such as DXA, ADP and US could be employed. Similarly, field methods such as anthropometry offer a cost-effective means of monitoring SAT, provided the operator has the necessary training. Clearly, BIA and the BMI are not supported for assessing or monitoring body composition, nor are those methods that make assumptions about the density of FFM in their computation.

Recent developments in US imaging have made possible accurate and reliable estimates of fat thickness in multiple sites of the body. However, interpretation of the obtained scan image is a difficult task and further research is necessary in this field. Many coaches and sport scientists anticipate the future development of a minimum sum of fat thickness, which corresponds to a minimum whole body % fat, for the establishment of participation standards for all athletic groups. While the available body composition methods do not permit this at present, some of the emerging medical imaging technologies may achieve the required accuracy to make this a reality in the future.

Regardless of the method favoured, it is imperative that coaches, athletes and scientists appreciate the importance necessarily attached to the presentation of an athlete for measurement. Their adherence to fundamental pre-requisites such as fasting, no exercise in the past 12-24 hours and standardization of hydration influences crucially the body composition data on which decisions are predicated. For instance, glycogen supercompensation can make a noticeable difference to skinfold compressibility, increase conductivity as a result of water storage, and add to fat-free soft tissue registered by a DXA scan. Altering fluid or electrolyte balance, which is an inevitable consequence of training and competition, will adversely affect measured body composition in several techniques, so standardization of athlete presentation prior to measuring is of paramount importance and should be the aspiration of national laboratories for high performance testing.

REFERENCES

1. Nattiv A, Loucks AB, Manore MM, et al. The female athlete triad special communications: Position Stand. *Med Sci Sports Exerc* 2007 39 (10): 1867-82
2. Sundgot-Borgen J, Torstveit MK. Aspects of disordered eating continuum in elite high-intensity sports. *Scand J Med Sci Sports* 2010 20:112–21
3. Müller W. Towards research based approaches for solving body composition in sports: ski jumping as a heuristic example. *Br J Sports Med* 2009 43 (13): 1013-19
4. Müller W. Determination of ski jump performance and implications for health, safety and fairness. *Sports Med* 2009 39 (2): 85-106
5. Müller W, Gröschl W, Müller R, et al. Underweight in ski jumping: the solution of the problem. *Int J Sports Med* 2006 27: 926-34
6. Adams J, Mottola M, Bagnell KM, et al. Total body fat content in a group of professional football players. *Can J Appl Sport Sci* 1982 7:36-40
7. Stewart AD, Hannan WJ. Prediction of fat and fat free mass in male athletes using dual X-ray absorptiometry as the reference method. *J Sports Sci* 2000 18:263-74
8. Hawse MR, Martin AD. Human body composition. In: Eston R, Reilly T, editors. *Kinanthropometry and exercise physiological laboratory manual: tests, procedures and data*, 2nd ed. London: Routledge, 2001: 7-43
9. Martin AD, Ross WD, Drinkwater DT, et al. Prediction of body fat by skinfold caliper: assumptions and cadaver evidence. *Int J Obesity* 1985 9: 31-9
10. Martin AD, Spenst LF, Drinkwater DT, et al. Anthropometric estimation of muscle mass in men. *Med Sci Sports Exer* 1990 22:729-33
11. Martin AD, Drinkwater DT, Clarys JP, et al. Effects of skin thickness and skinfold compressibility on skinfold thickness measurement. *Am J Hum Biol* 1992 4(4): 453-60
12. Wang Z, Shen W, Withers RT, et al. Multicomponent molecular-level models of body composition analysis. In: Heymsfield SB, Lohman TG, Wang ZM, et al., editors. *Human body composition: 2nd ed.* Champaign (IL): Human Kinetics, 2005: 163-76
13. Withers RT, Laforgia J, Heymsfield SB. Critical appraisal of the estimation of body composition via two-, three-, and four-compartment models. *Am J Hum Biol* 1999 11 (2): 175-85
14. Friedl KE, DeLuca JP, Marchitelli LJ, et al. Reliability of body-fat estimations from a four-component model by using density, body water, and bone mineral measurements. *Am J Clin Nutr* 1992 55: 764-70
15. Lohman TG, Harris M, Teixeira PJ, et al. Assessing body composition and changes in body composition. Another look at dual-energy X-ray absorptiometry. *Ann N Y Acad Sci* 2000 904: 45-54

16. Clasey JL, Kanaley JA, Wideman L, et al. Validity of methods of body composition assessment in young and older men and women. *J Appl Physiol* 1999 86 (5): 1728-38
17. Wang Z, Heymsfield SB, Chen S, et al. Estimation of percentage body fat by dual-energy x-ray absorptiometry: evaluation by in vivo human elemental composition. *Phys Med Biol* 2010 55: 2619-35
18. Runge VM, Nitz WR, Schmeets SH. *The physics of clinical MR: taught through images*. New York: Thieme, 2005
19. Liang Z-P, Lauterbur PC. *Principles of magnetic resonance imaging. A signal processing perspective*. New York: IEEE Press, 2000
20. Clarys JP, Scafoglieri A, Provyn S, et al. A macro-quality evaluation of DXA variables using whole dissection, ashing and computer tomography in pigs. *Obesity* 2010 18(8): 1477-85
21. Pietrobelli A, Formica C, Wang Z, et al. Dual-energy X-ray absorptiometry body composition model: review of physical concepts. *Am J Physiol* 1996 271: E941-51
22. Prior BM, Cureton KJ, Modelsky CM, et al. In vivo validation of whole body composition estimates from dual-energy X-ray absorptiometry. *J Appl Physiol* 1997 83: 623-30
23. Wang ZM, Visser M, Ma R, et al. Skeletal muscle mass: evaluation of neutron activation and dual-energy x-ray absorptiometry methods. *J App Physiol* 1996 80 (3): 824-31
24. Wang W, Wang Z, Faith MS, et al. Regional skeletal muscle measurement: evaluation of new dual-energy X-ray absorptiometry model. *J App Physiol* 1999 87 (3): 1163-71
25. Kim J, Wang Z, Heymsfield SB, et al. Total-body skeletal muscle mass: estimation by a new dual-energy X-ray absorptiometry method. *Am J Clin Nutr* 2002 76 (2): 378-83
26. Tothill P, Hannan WJ, Wilkinson S. Comparisons between a pencil beam and two fan beam dual energy X-ray absorptiometers used for measuring total body bone and soft tissue. *Brit J Radiol* 2001 74: 166-76
27. Visser V, Fuerst T, Lang T, et al. Validity of fan beam dual-energy X-ray absorptiometry for measuring fat-free mass and leg muscle mass. *J App Physiol* 1999 87 (4): 1513-20
28. Brozek J, Grande F, Anderson JT, et al. Densitometric analysis of body composition: revision of some quantitative assumptions. *Ann NY Acad Sci* 1963 110: 113-40
29. Siri WE. The gross composition of the body. In: Lawrence JH, Tobias CA, editors. *Advances in biological and medical physics*. London: Academic Press, 1956
30. Going SB. Hydrodensitometry and air displacement plethysmography. In: Heymsfield SB, Lohman TG, Wang ZM, et al., editors. *Human body composition*, 2nd ed. Champaign (IL): Human Kinetics, 2005:17-33
31. Wilmore JH, Vodak PA, Parr RB, et al. Further simplification of a method for determination of residual volume. *Med Sci Sports Exerc* 1980 12: 216-8

32. Peeters M, Claessens A. Effect of deviating clothing schemes on the accuracy of body composition measurements by air-displacement plethysmography. *Inte J Body Comp Res* 2009 7 (4): 123-9
33. Peeters M, Claessens A. Effect of different swim caps on the assessment of body volume and percentage body fat by air displacement plethysmography. *J Sports Sci* 2011 29: 191-6
34. Biaggi RB, Vollman MW, Niles MA, et al. Comparison of air-displacement plethysmography with hydrostatic weighing and bioelectrical impedance analysis for the assessment of body composition in healthy adults. *Am J Clin Nutr* 1999 69: 898-903
35. Vescovi J, Hildebrandt L, Miller W, et al. Evaluation of the BOD POD for estimating percent fat in female college athletes. *J Str Cond Res*, 2002 16: 599-605
36. Claros G, Hull HR, Fields DA. Comparison of air displacement plethysmography to hydrostatic weighing for estimating total body density in children. *BMC Pediatrics* 2005 5: 37
37. Collins MA, Millard-Stafford ML, Sparling PB, et al. Evaluation of the BOD POD for assessing body fat in collegiate football players. *Med Sci Sports Exerc* 1999 31(9):1350-6
38. Bender DA, Bender AE. *Nutrition: A reference handbook*. Oxford: Oxford University Press, 1997: 10-138
39. Institute of Medicine. *Dietary reference intakes for water, sodium, chloride, potassium and sulphate*. Washington DC: National Academic Press, 2005: 73-185
40. Schoeller DA. Hydrometry. In: Heymsfield SB, Lohman TG, Wang ZM, et al., editors. *Human body composition*, 2nd ed. Champaign (IL): Human Kinetics, 2005: 35-49
41. Bullen BA, Quaade F, Olsen F, et al. Ultrasonic reflections used for measuring subcutaneous fat in humans. *Hum Biol* 1965 37 (4): 375-84
42. Booth RAD, Goddard BA, and Paton A. Measurement of fat thickness in man: a comparison of ultrasound, Harpenden calipers and electrical conductivity. *Brit J Nutr* 1966 20 (4): 719-25
43. Bellisari A, Roche AF. Anthropometry and ultrasound. In: Heymsfield SB, Lohman TG, Wang ZM, Going SB, editors. *Human body composition*. 2nd ed. Champaign (IL): Human Kinetics, 2005: 109-27
44. Bellisari A, Roche AF, Siervogel RM. Reliability of B-mode ultrasonic measurements of subcutaneous adipose tissue and intra-abdominal depth: comparisons with skinfold thickness. *Int J Obes Relat Metab Disord* 1993 17 (8): 475-80
45. Ishida Y, Carroll JF, Pollock ML, et al. Reliability of B-mode ultrasound for the measurement of body fat and muscle thickness. *Am J Hum Biol* 1992 4: 511-20
46. Abe T, Kawakami Y, Sugita M, Yoshikawa K, et al. Use of B-mode ultrasound for visceral fat mass evaluation: comparisons with magnetic resonance imaging. *Appl Human Sci* 1995 14 (3): 133-9

47. Moore TL, Lunt M, McManus B, et al. Seventeen-point dermal ultrasound scoring system – a reliable measure of skin thickness in patients with systemic sclerosis. *Rheumatology* 2003 42 (12): 1559-63
48. Horn M, Müller W. Towards an accurate determination of subcutaneous adipose tissue by means of ultrasound [abstract WCB-A01448-02611]. 6th World Congress of Biomechanics; 2010; Singapore
49. Ross R, Janssen I. Computed tomography and magnetic resonance imaging. In: Heymsfield SB, Lohman TG, Wang ZM, et al., editors. *Human body composition*, 2nd ed. Champaign (IL): Human Kinetics, 2005: 89-108
50. Koda M, Senda M, Kamba M, et al. Subcutaneous and visceral fat indices represent the distribution of body fat volume. *Abdom Imaging* 2007 32 (3): 387-92
51. Wells JCK, Treleaven P, Cole TJ. BMI compared with 3-dimensional body shape: The UK national sizing survey. *Am J Clin Nutr* 2007 85: 419-25
52. Wells JCK, Cole TJ, Treleaven P. Age-variability in body shape associated with excess weight: The UK national sizing survey. *Obesity* 2008 16: 435-41
53. Wells JCK, Cole TJ, Bruner D, et al. Body shape in American and British adults: between-country and inter-ethnic comparisons. *Int J Obesity* 2008 32: 152-59
54. Wang J, Gallagher D, Thornton JC, et al. Validation of a 3-dimensional photonic scanner for the measurement of body volumes, dimensions, and percentage body fat. *Am J Clin Nutr* 2006 83: 809-16
55. Garlie TN, Obusek JP, Corner BD, et al. Comparison of body fat estimates using 3D digital laser scans, direct manual anthropometry and DXA in men. *Am J Hum Biol* 2010 22: 695-701
56. Schranz N, Tomkinson G, Olds T, et al. Three-dimensional anthropometric analysis: Differences between elite Australian rowers and the general population. *J Sports Sci* 2010 28: 459-69
57. Mateigka J. The testing of physical efficiency. *Am J Phys Anthropol* 1921 4: 223–30
58. Tanner JM. *The physique of the Olympic athlete*. London: George Allen & Unwin Ltd, 1964
59. Lohman TG, Roche AF, Martorell R. *Anthropometric standardization reference manual*. Champaign (IL): Human Kinetics, 1988
60. Hume P, Marfell-Jones M. The importance of accurate site location for skinfold measurement. *J Sports Sci* 2008 26: 1333-40
61. Marfell-Jones M, Olds T, Stewart AD, et al. International standards for anthropometric assessment. Potchesfstrom: International Society for the Advancement of Kinanthropometry, 2006

62. Durnin JVGA, Womersley J. Body fat assessed from total body density and its estimation from skinfold thickness: Measurements on 481 men and women aged 16 to 72 years. *Br J Nutr* 1974 32: 77-97
63. Sinning WE, Dolny DG, Little KD, et al. Validity of “generalised” equations for body composition analysis in male athletes. *Med Sci Sports Exerc* 1985 17: 124-30
64. Thorland WG, Tipton CM, Lohman TG, et al. Midwest wrestling study: prediction of minimal weight for high school wrestlers. *Med Sci Sports Exerc* 1991 23 (9): 1102-10
65. Lohman TG. Skinfolts and body density and their relationship to body fatness: a review. *Hum Biol* 1981 53 (2): 181-255
66. Behnke AR, Wilmore JH. Evaluation and regulation of body build and composition. Englewood Cliffs NJ: Prentice Hall, 1974
67. Van Der Kooy K, Leenen R, Siedell JC, et al. Abdominal diameters as indicators of visceral fat: comparison between magnetic resonance imaging and anthropometry. *Brit J Nutr* 1993 70: 47-58
68. Valsamakis G, Chetty R, Anwar A, et al. Association of simple anthropometric measures of obesity with visceral fat and the metabolic syndrome. *Diabetic Med* 2004 21: 1339-448
69. Iribarren C, Darbinian JA, Lo JC, et al. Value of the sagittal abdominal diameter in coronary heart disease risk assessment: Cohort study in a large, multiethnic population. *Am J Epidemiol* 2006 164: 1150-9
70. Stewart AD, Nevill AM, Johnstone AM. Shape change assessed by 3D laser scanning following weight loss in obese men. In: Hume P, Stewart AD, de Ridder H, editors. *Kinanthropometry XI: 2008 Pre-Olympic Congress Anthropometry Research*. Auckland: Auckland University of Technology, 2009: 20-4
71. Marfell-Jones MJ. The value of the skinfold – background assumptions, cautions, and recommendations on taking and interpreting skinfold measurements. In: *KAHPERD, Proceedings of the 2001 Seoul International Sport Science Congress, Seoul, Korea. 2001: 313-23*
72. Carter JEL. Morphological factors limiting human performance. In: Eckert HM, Clarke DH, editors. *The limits of human performance. The American Academy of Physical Education Papers, No. 18. Champaign (IL): Human Kinetics, 1985: 106-17*
73. Carter JEL, Ackland TR. *Kinanthropometry in Aquatic Sports*. Champaign IL: Human Kinetics Publishers, 1994
74. Ridge BR, Broad E, Kerr DA, Ackland TR. Morphological characteristics of Olympic slalom canoe and kayak paddlers. *Europ J Sp Sci*, 2007 7(2): 107-13
75. Kerr DA, Ackland TR, Ross WD, et al. Olympic lightweight and open rowers possess distinctive physical and proportionality characteristics. *J Sp Sci* 2007 25(1): 43-53

76. Carter JEL, Ackland TR, Kerr DA, Stapff AB. Somatotype and size of elite female basketball players. *J Sp Sciences* 2005 23(10): 1057-63
77. Kerr DA, Stewart AD. Body composition in sport. In: Ackland T, Elliott B, Bloomfield J, editors. *Applied anatomy and biomechanics in sport*. Champaign (IL): Human Kinetics, 2009: 67-86
78. Orphanidou CI, McCargar LJ, Birmingham CL, et al. Changes in body composition and fat distribution after short term weight gain in patients with anorexia nervosa. *Am J Clin Nutr* 1997 65: 1034-41
79. Stewart AD. Anthropometric fat patterning in male and female subjects. In: Reilly T, Marfell-Jones M, editors. *Kinanthropometry VIII: Proceedings of the 8th International Society for the Advancement of Kinanthropometry Conference*. London: Routledge 2003: 195-238.
80. Stewart AD. Unpublished PhD thesis entitled *Body composition in athletes assessed by DXA and other methods*. University of Edinburgh, 1999
81. Chumlea WC, Sun SS. Bioelectrical impedance analysis. In: Heymsfield SB, Lohman TG, Wang ZM, et al., editors. *Human body composition*, 2nd ed. Champaign (IL): Human Kinetics, 2005: 79-87
82. Matthie JR. Bioimpedance measurements of human body composition: critical analysis and outlook. *Expert Rev Med Devices* 2008 5 (2): 239-61
83. Wabel P, Chamney P, Moissl U, et al. Importance of whole-body bioimpedance spectroscopy for the management of fluid balance. *Blood Purif* 2009 27 (1): 75-80
84. Lohman TG, *Advances in human body composition*. Champaign (IL): Human Kinetics Publishers, 1992
85. Lee J, Kolonel LN, Hinds MW. Relative merits of the weight-corrected-for-height indices. *Am J Clin Nutr* 1981 34: 2521-9
86. Keyes A, Fidanza F, Karvonen MJ, et al. Indices of relative weight and obesity. *J Chron Dis* 1972 25: 329-43
87. Benn RT. Some mathematical properties of weight-for-height indices used as measures of adiposity. *Br J Prev Soc Med* 1971 25: 42-50
88. WHO Expert Committee. *Physical status, use and interpretation of anthropometry*. Technical Report Series 1995 854: 355
89. Norgen NG. Population differences in body composition in relation to the BMI. *Eur Clin Nutr* 1994 48: 10-27
90. Nevill AM, Winter EM, Ingham SA, et al. Adjusting athletes' body mass index to better reflect adiposity in epidemiological research. *J Sp Sci* 2010 28: 1009-24

91. WHO Expert Committee. Physical status, use and interpretation of anthropometry. Technical Report Series 1995; 854:428

List of Tables

Table I. Features of body composition reference methods

Table II. Features of body composition laboratory methods

Table III. Features of body composition field methods

Table I. Features of body composition reference methods

Method	Level ¹	Approach	Comp ²	Outcome Measures	Assumptions / cautions	Advantages	Limitations
Cadaver dissection	D	Anatomical	5	Tissue masses: <ul style="list-style-type: none"> • Skin • Adipose • Bone • Muscle • Other 	<ul style="list-style-type: none"> • Limited number of dissected specimens cannot be representative of the range of body types and compositions among athletes 	<ul style="list-style-type: none"> • May be used to validate other indirect methods 	<ul style="list-style-type: none"> • Small numbers of cadavers • None were athletic • Limited range of structures • Long and tedious method • Loss of body fluid • Cannot be used for individual analysis
Multicomponent models	D	Chemical	3-6	<ul style="list-style-type: none"> • Fat mass • Body density • Total body water • Bone mineral • Protein 	<ul style="list-style-type: none"> • Bone mineral includes other mineral in other tissues • Constant proportion of protein to water • Assume constant densities of each component 	<ul style="list-style-type: none"> • Most appropriate reference method to date • Accommodates variability of both bone mineral and water content which invalidates the two component model. 	<ul style="list-style-type: none"> • Long analysis process • Expensive technology • Lack of published normative data
Medical imaging: MRI and CT ³	D	Anatomical	4	Tissue thickness/ area/volume: <ul style="list-style-type: none"> • Adipose • Bone • Muscle • Other 	<ul style="list-style-type: none"> • Both machines designed primarily for diagnostic use rather than quantifying tissue dimensions • Relating anatomical dimensions to tissue masses requires assumptions about tissue densities • More assumptions and vast computing power required for in assessing deep fat depots 	<ul style="list-style-type: none"> • No exposure to ionizing radiation with MRI 	<ul style="list-style-type: none"> • Expensive technology • Long analysis process • High exposure to ionizing radiation with CT • Confined space of some apparatus may induce claustrophobia • Lack of published normative data

Note: 1. Levels of analysis; D = direct, I = indirect, DI = doubly indirect
2. Comp = number of components.
3. MRI = magnetic resonance imaging, CT = computed tomography

Table II. Features of body composition laboratory methods

Method	Level ¹	Approach	Comp ²	Outcome Measures	Assumptions / cautions	Advantages	Limitations
DXA ³	D	Chemical	3	Component mass: <ul style="list-style-type: none"> • Fat (lipid) • Bone mineral • Other fat free soft tissue 	<ul style="list-style-type: none"> • Interpolation for soft tissues in areas where bone is detected • Assumes magnification errors and beam hardening are insignificant 	<ul style="list-style-type: none"> • Whole body approach • Cost and time efficiency • Minimal subject action needed • Small radiation dose • Minimal operator training • Regional compartment analysis • Independent of hydration status • Good precision • Validation against porcine models 	<ul style="list-style-type: none"> • Calculation algorithms differ between manufacturers and are not published • Pencil versus fan beam differences in accuracy • Limited scan bed size • Cannot scan if pregnant • Regional legislative requirements differ
Densitometry-(UWW)	D	Chemical	0	Whole body density	<ul style="list-style-type: none"> • UWW requires estimation of residual volume and other entrapped air spaces 	<ul style="list-style-type: none"> • Whole body approach 	<ul style="list-style-type: none"> • UWW requires considerable subject involvement • Requirement to remain still throughout and issues of water confidence create difficulties for measuring children • Estimation of entrapped air spaces is problematic • Body density does not provide information about individual tissue components
Densitometry-(UWW)	I	Chemical	2	<ul style="list-style-type: none"> • % Fat • % Fat-free 	<ul style="list-style-type: none"> • Uses invalid assumptions regarding the density of fat-free tissues 	<ul style="list-style-type: none"> • Whole body approach • Simple calculation 	<ul style="list-style-type: none"> • Method not supported in strength trained individuals and other populations including osteoporotic, children and athletes
Densitometry-(ADP)	I	Chemical	2	<ul style="list-style-type: none"> • % Fat • % Fat-free 	<ul style="list-style-type: none"> • ADP makes assumptions about the thermal air properties within the chamber • ADP requires estimate of other entrapped air spaces • Uses invalid assumptions regarding the density of fat-free tissues 	<ul style="list-style-type: none"> • ADP is easier to administer, is more time efficient and requires less participant action and/or discomfort than UWW • Does not require water confidence • Simple calculation 	<ul style="list-style-type: none"> • Requirement to remain still throughout creates difficulties for measuring children • Method not supported in strength trained individuals and other populations including osteoporotic, children and athletes
Hydrometry-(Body water)	D	Chemical	0	<ul style="list-style-type: none"> • % water 	<ul style="list-style-type: none"> • The tracer is distributed homogeneously equally across all components and is not metabolised 	<ul style="list-style-type: none"> • Whole body approach • Minimal subject action needed • Can use saliva, urine or blood to estimate the dilution • Easy to administer 	<ul style="list-style-type: none"> • Time to reach equilibrium (3-4 hours) • Expensive • Acute ingestion of a large bolus of fluid affects the assessment

Hydrometry- (Body water)	D	Chemical	2	<ul style="list-style-type: none"> • % Fat • % Fat-free 	<ul style="list-style-type: none"> • Uses invalid assumptions regarding the hydration of fat-free tissues 	<ul style="list-style-type: none"> • Easy to administer 	<ul style="list-style-type: none"> • Method not supported in people with cardiac, kidney disease and those with oedema and other fluid retention problem
Ultrasound	D	Anatomical	3	Tissue layer thickness <ul style="list-style-type: none"> • Skin • Adipose • Muscle 	<ul style="list-style-type: none"> • No image distortion • Correct speed of sound used for given tissue • Correct detection of tissue layer boundaries 	<ul style="list-style-type: none"> • High accuracy and precision • Applicable in the field • Non-invasive and no ionising radiation • No tissue compression • Tissue thickness from 1 mm to 300 mm measureable • Many thickness measurements from each image • Rapid data acquisition • Minimal subject involvement • Low cost compared to MRI or CT 	<ul style="list-style-type: none"> • Samples the subcutaneous fat deposit only • Considerable skill necessary • Method is not standardised yet • Ultrasound technique includes inherent artefacts
3D photonic scanning	D	Anatomical	0	<ul style="list-style-type: none"> • Body surface area • Body volume • Shape parameters 	<ul style="list-style-type: none"> • Clothing tightness does not affect the body's contour or profile • Always overestimates body volume due to hair or clothing 	<ul style="list-style-type: none"> • Minimum subject involvement • Rapid data acquisition (10-15 s) 	<ul style="list-style-type: none"> • Some clothing colours and textures affect image quality • Hirsutism affects body volume
3D photonic scanning	I	Chemical	2	<ul style="list-style-type: none"> • % Fat • % Fat-free 	<ul style="list-style-type: none"> • Uses invalid assumptions regarding the density of FM and FFM 	<ul style="list-style-type: none"> • As above 	<ul style="list-style-type: none"> • Method not supported in strength trained individuals and other populations including osteoporotic, children and athletes

- Note:
1. Levels of analysis; D = direct, I = indirect, DI = doubly indirect
 2. Comp = number of components.
 3. DXA = dual energy X-ray absorptiometry, UWW = underwater weighing, ADP = air displacement plethysmography, 3D = three dimensional

Table III. Features of body composition field methods

Method	Level ¹	Approach	Comp ²	Outcome Measures	Assumptions / cautions	Advantages	Limitations
Anthropometry- (Skinfolds)	I	Anatomical	1	<ul style="list-style-type: none"> • Skinfold sum • Skinfold ratios 	<ul style="list-style-type: none"> • Consistent fat patterning • Fixed subcutaneous to internal fat relationship • Constant skinfold compressibility • Constant skin to adipose fraction • Lipid fraction of adipose tissue • Water content of adipose tissue 	<ul style="list-style-type: none"> • Reliable scores with trained technicians • Results can be compared with norms • Legitimate for test re-test on individuals • Low cost, convenient data collection 	<ul style="list-style-type: none"> • Samples the subcutaneous fat deposit only • Can be intrusive for some individuals • Some sites difficult to achieve • Standardization of method essential
Anthropometry- (Skinfolds equations)	DI	Anatomical	2	<ul style="list-style-type: none"> • % Fat • % Fat-free 	<ul style="list-style-type: none"> • Aggregates the limitations of both dependent and independent variables in the prediction equation 	<ul style="list-style-type: none"> • Method has some applicability with some populations 	<ul style="list-style-type: none"> • Numerous equations available which can cause confusion • Method not supported in extreme populations (e.g. the obese) • Equations are population-specific and need to be cross-validated for the sample in question
BIA	I	Chemical	2	<ul style="list-style-type: none"> • Total body water • % Fat • % Fat-free 	<ul style="list-style-type: none"> • Assumes subject compliance to testing prerequisites • Assumes geometric similarity between individuals • Assumes tissue resistivity is similar between individuals • Input data (age, height, weight, athletic status) accounts for high (up to 85%) of variance in the dependent variable 	<ul style="list-style-type: none"> • Precision high • Minimal subject involvement • No ionising radiation • Minimum subject involvement • Rapid data acquisition • Apparent sophistication 	<ul style="list-style-type: none"> • Accuracy poor • Results affected by hydration status • Trunk underrepresented / limbs overrepresented in value • Several different models have electrodes places at various positions on the body (arm to leg, leg to leg, arm to arm)
BMI and MI	I	Anatomical	0	Index of relative weight (ponderosity)	<ul style="list-style-type: none"> • Assumes weight change is related solely to adiposity • Fat free mass to height proportion is constant • Assumes constant body segment proportions 	<ul style="list-style-type: none"> • Precision high • Minimal subject involvement • Minimum subject involvement • Rapid data acquisition 	<ul style="list-style-type: none"> • Great variability in fat content among individuals with the same BMI • Frame size, proportions and muscularity independently influence BMI • Mass and stature exhibit considerable diurnal variability

Note: 1. Level of analysis; D = direct, I = indirect, DI = doubly indirect
 2. Comp = number of components.
 3. BIA = bioelectrical impedance analysis, BMI = body mass index, MI = mass index

Figure 1

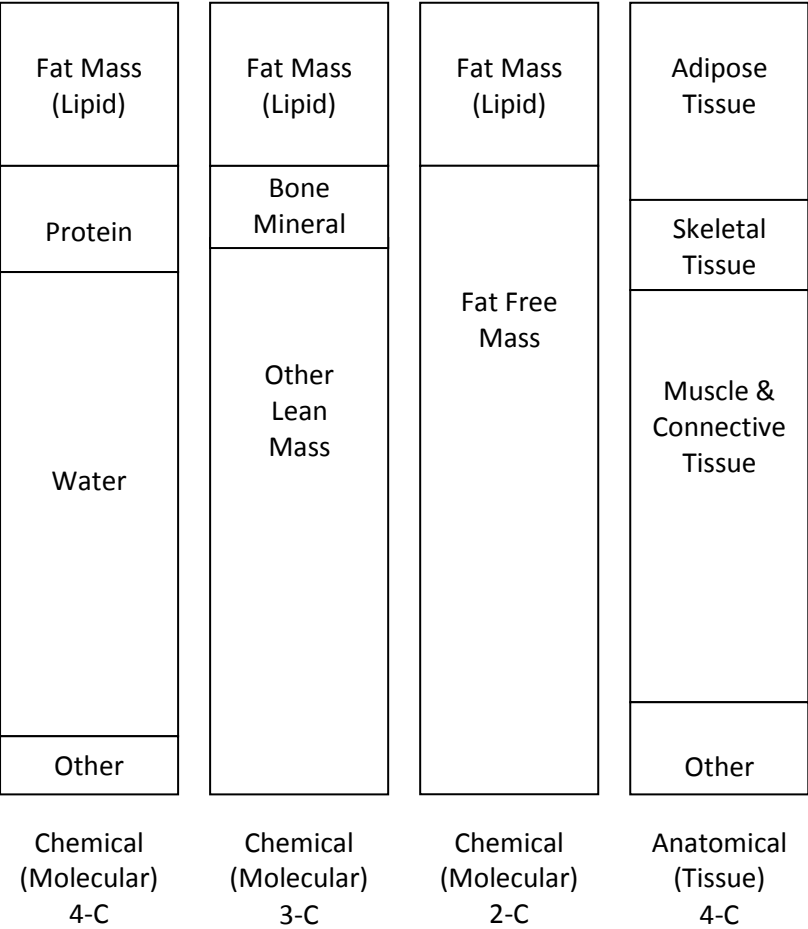


Figure 2

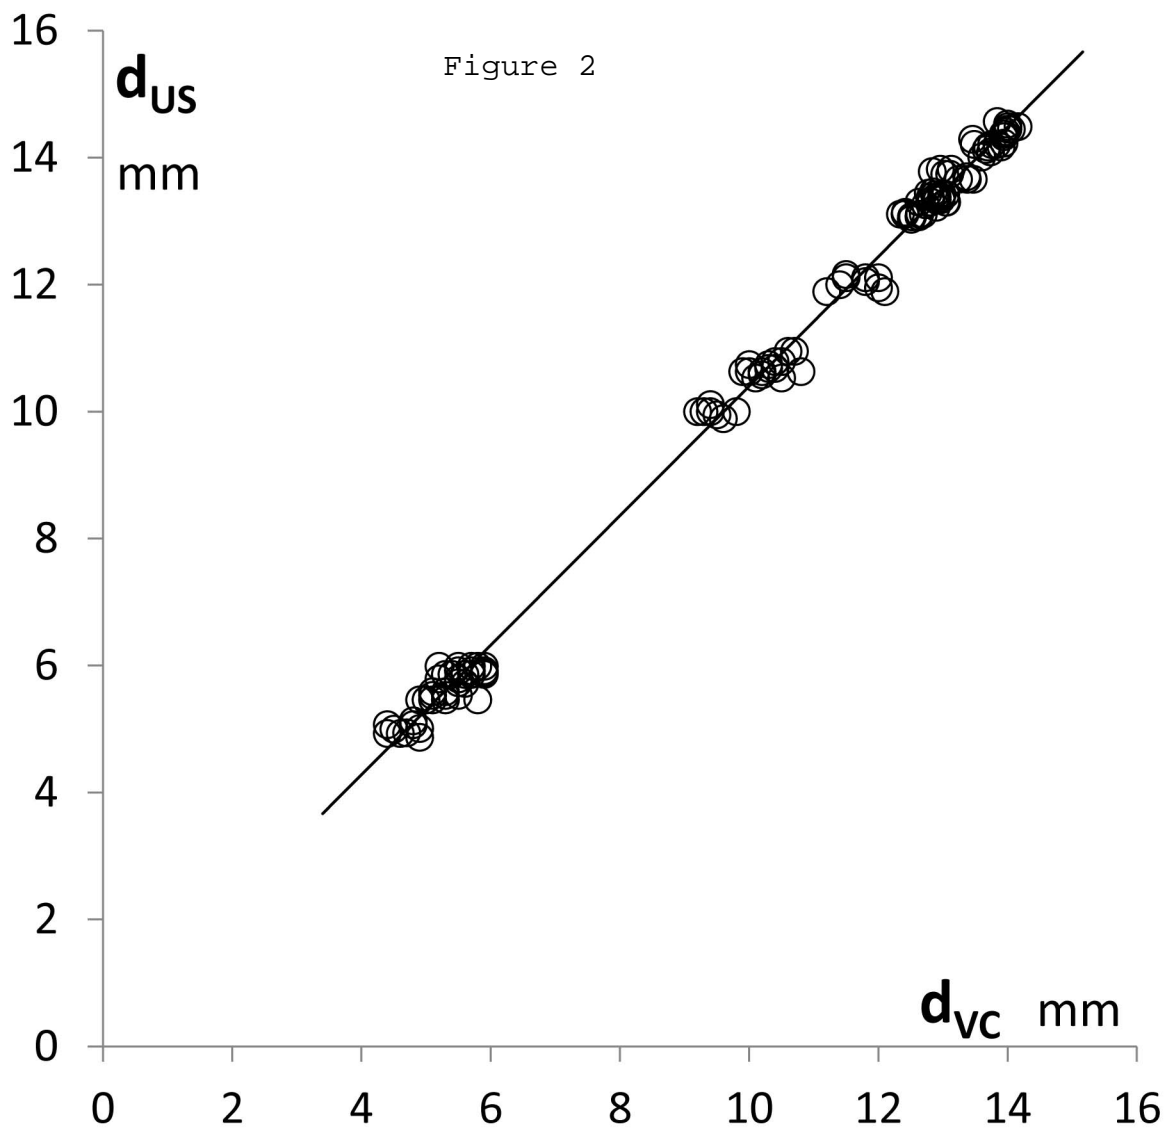


Figure 3

